

COLLAR® Papillary Muscle Exposure Device

Addresses the difficulty of inadequate exposure while placing sutures in the papillary muscles during MICS procedures.



EFFICIENT INSERTION

Available in two different sizes (small and large) to accommodate anatomical variances.



Material flexibility allows the device to be rolled for efficient insertion.



Directional arrow markers indicate proper orientation for insertion.


ENHANCED STABILIZATION AND TRACTION

Lateral Wings (A)

Unique bi-furcated tip geometry and material flexibility enable optimal wing positioning.


Inferior flange (B) and traction raisings (C)

Facilitate tissue engagement to enhance device stability within the mitral valve annulus.

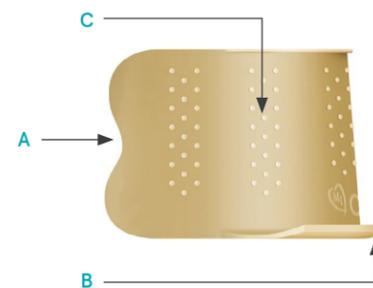


Material Flexibility

Facilitates optimal positioning and enhances device stabilization during mitral valve leaflet retraction.

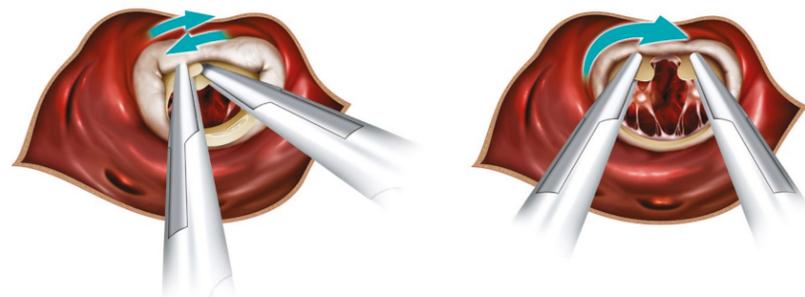

MAXIMIZED ACCESS AND EXPOSURE

Superior stiffening rib and material shape retention memory provide significant circumferential leaflet retraction to maximize intra-ventricular access and exposure.

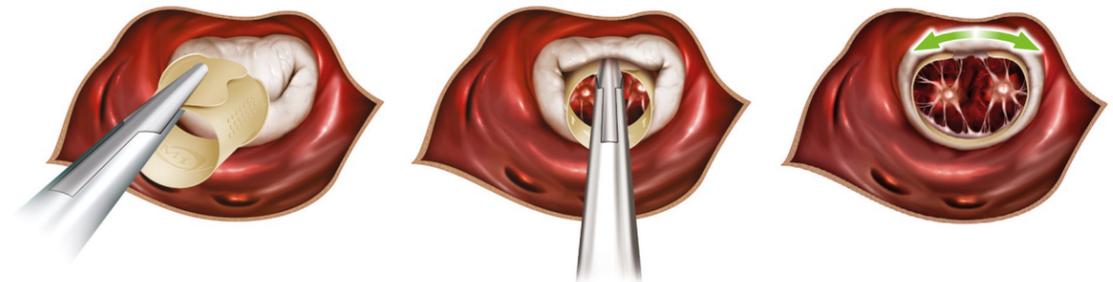

Ordering Information

Order #	Description
MI-COTIE-001	Box of 6 sterile pouches 2 Sizes COLLAR PAPILLARY MUSCLE EXPOSURE DEVICE per sterile pouch

Device Specifications

Description	A (cm)	B (cm)
COLLAR PAPILLARY MUSCLE EXPOSURE DEVICE (Small)	2.3	9
COLLAR PAPILLARY MUSCLE EXPOSURE DEVICE (Large)	3	11



INDICATIONS: The COLLAR device is intended for use to retract valve leaflet tissue during specific cardiac surgical procedures.

CONTRAINDICATIONS: None known.

WARNINGS AND PRECAUTIONS: This device is designed for single patient use only. Do not reuse, reprocess, or resterilize this product. Reuse, reprocessing, or resterilization may compromise the structural integrity of the device and/or create a risk of contamination of the device, which could result in patient injury, illness, or death. Do not use if package or product is damaged. It is the responsibility of the user to dispose of the device in accordance with local regulations and hospital procedures.

For additional information please refer to the Instructions for Use provided with the product.

CAUTION: Federal law (USA) restricts this device to sale by or on the order of a physician.